

FIG. 1A

102290 95646860

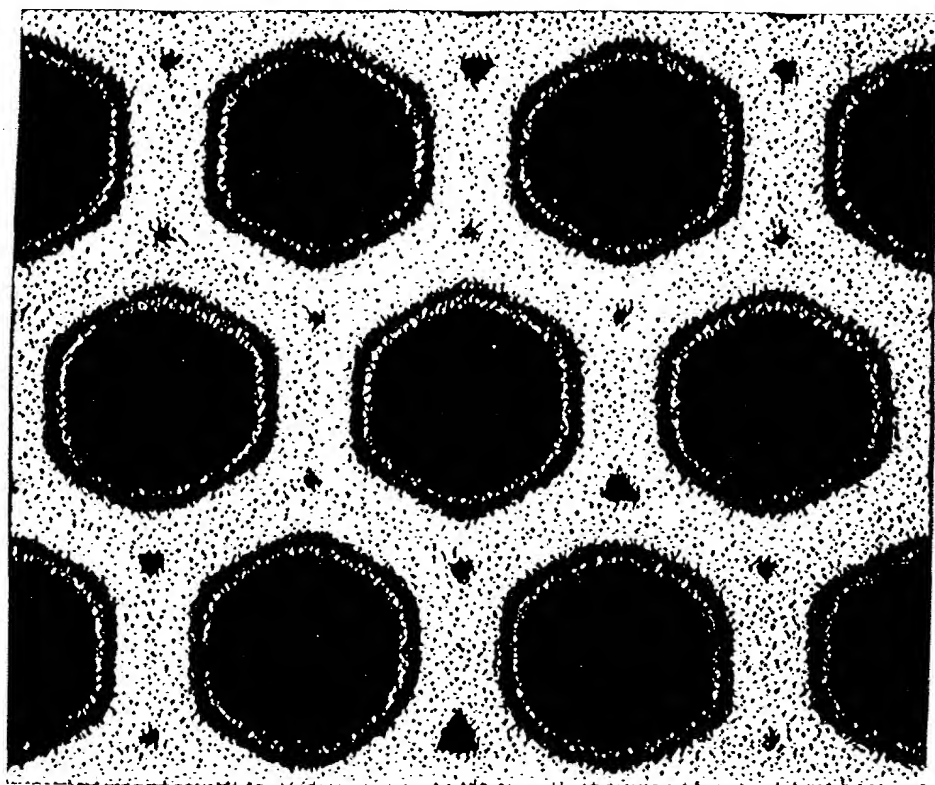


FIG. 1B

107290 95646860

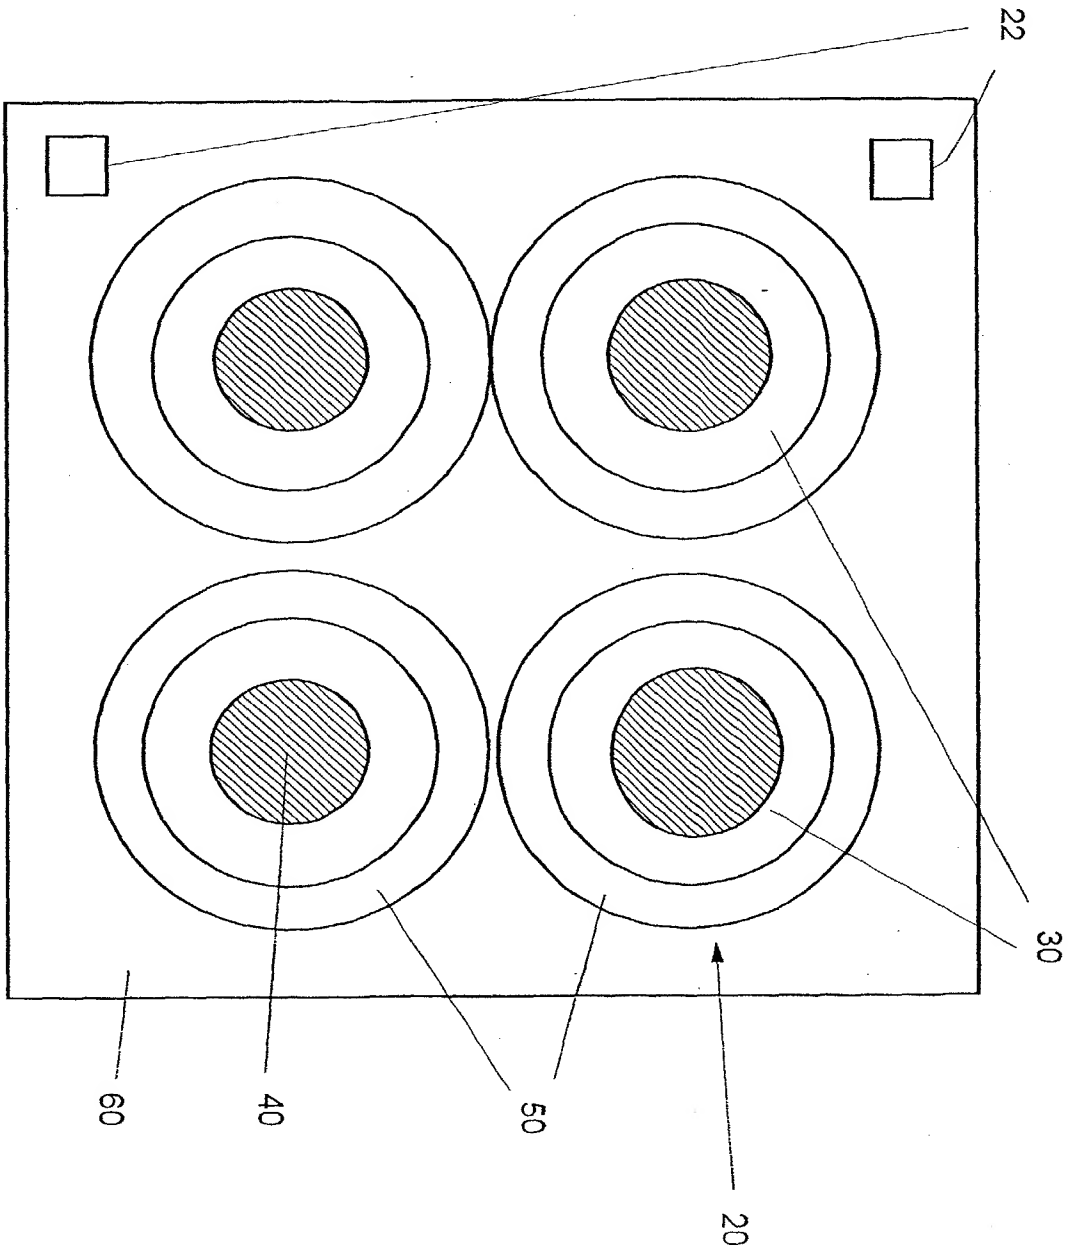


FIG. 2

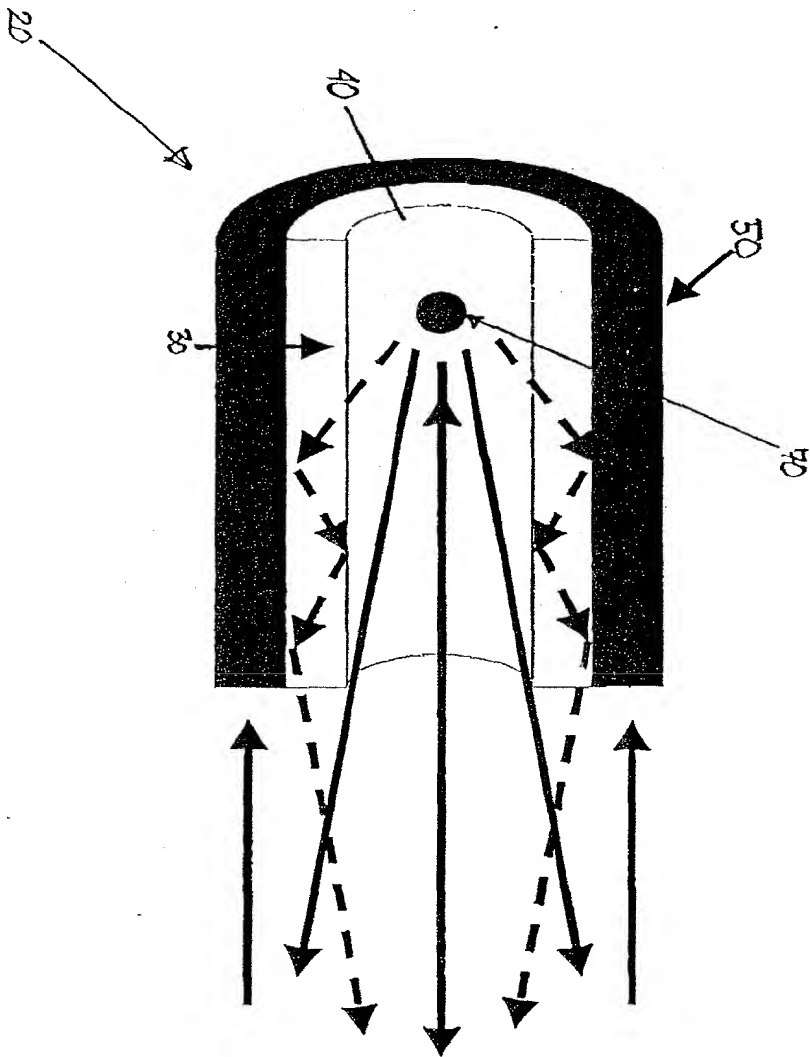


FIG. 3

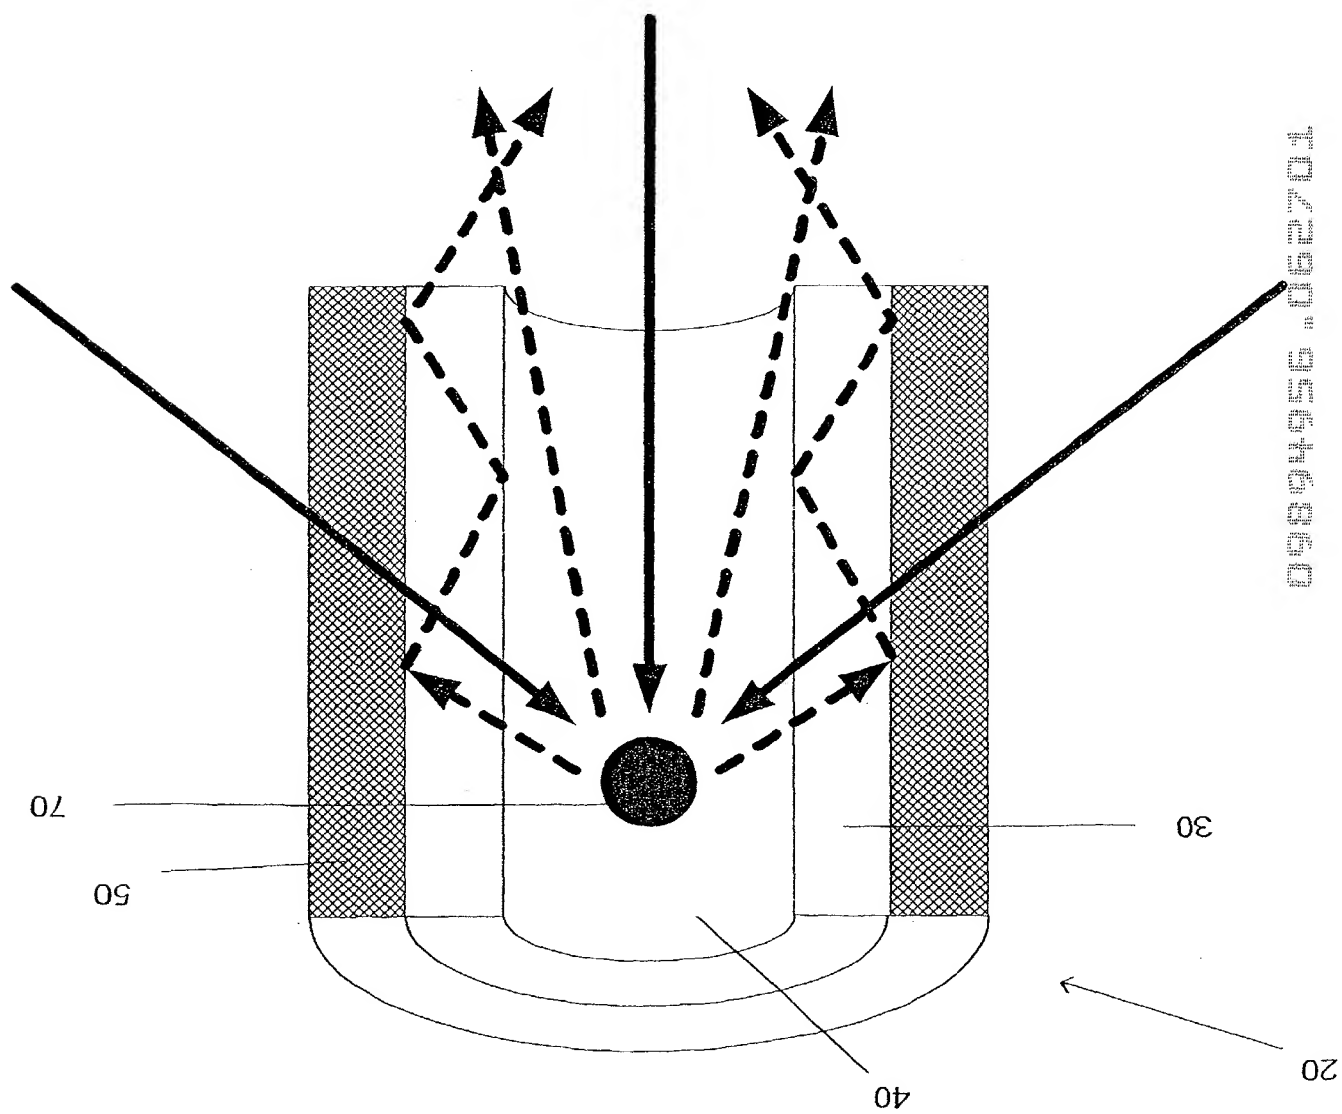


FIG. 4

102290 95646860

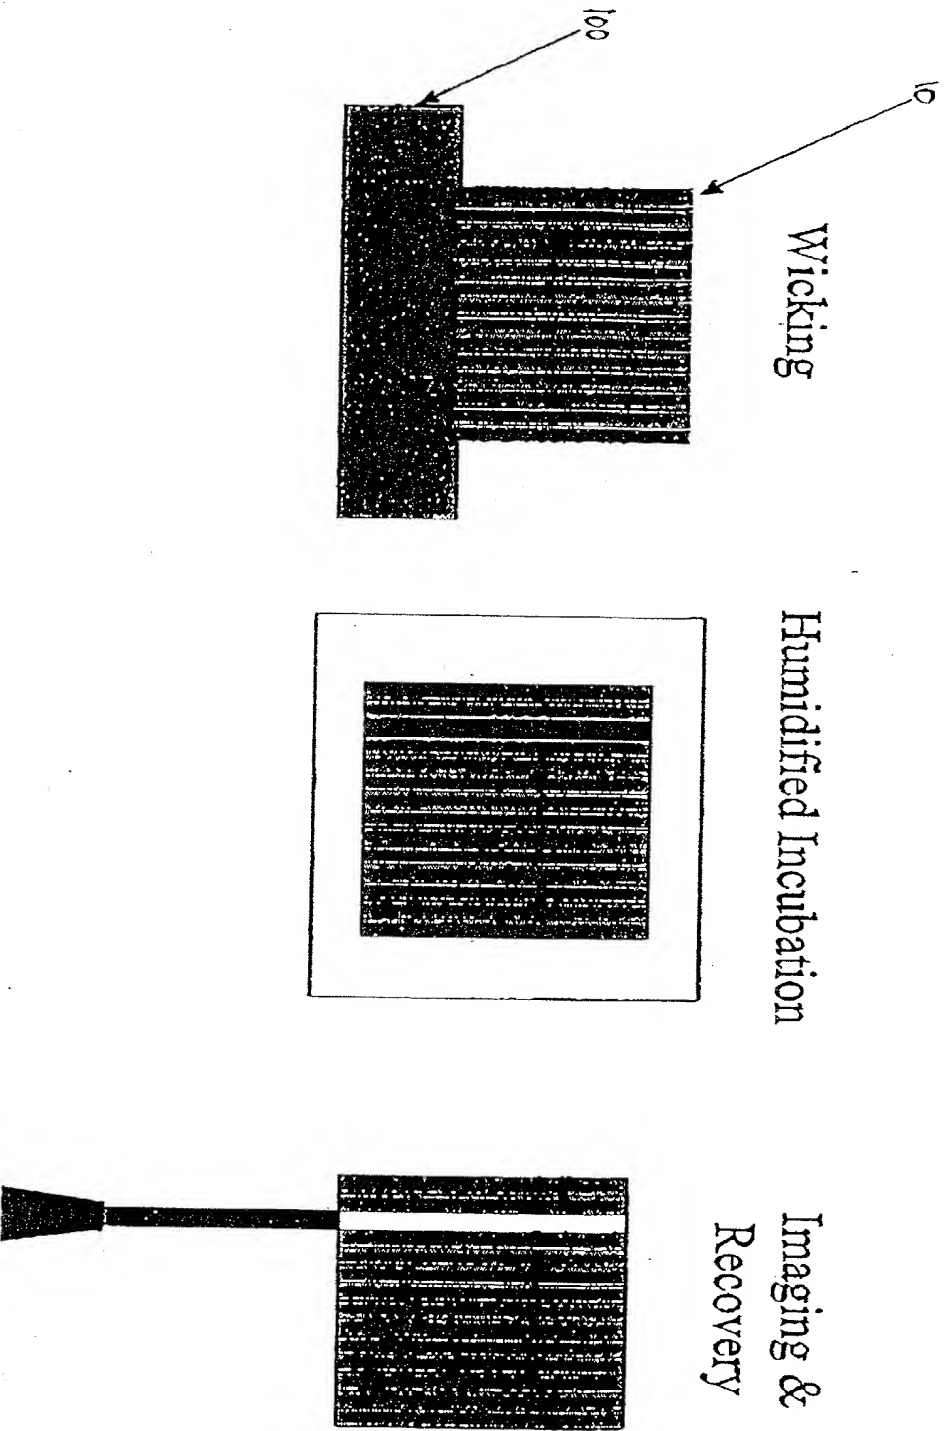


FIG. 5

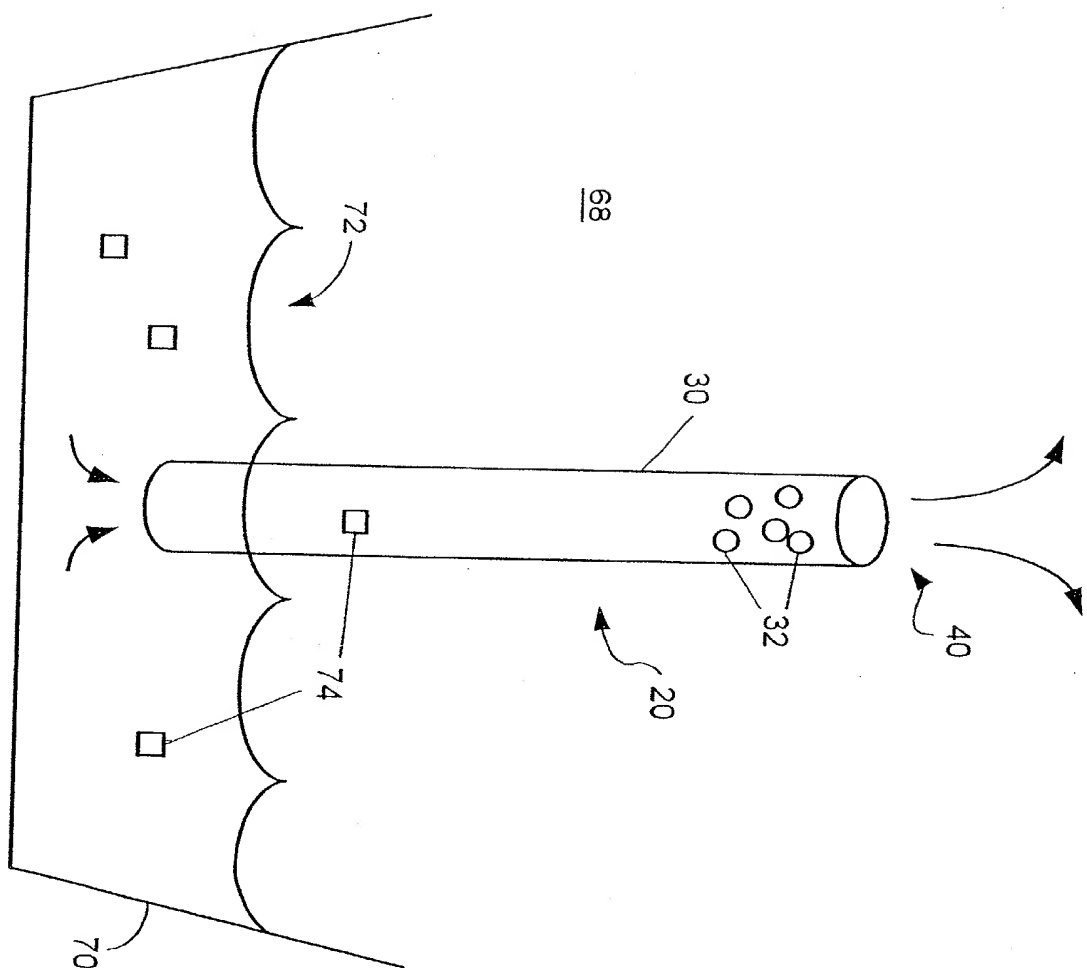


FIG. 6

10,2290 95646860

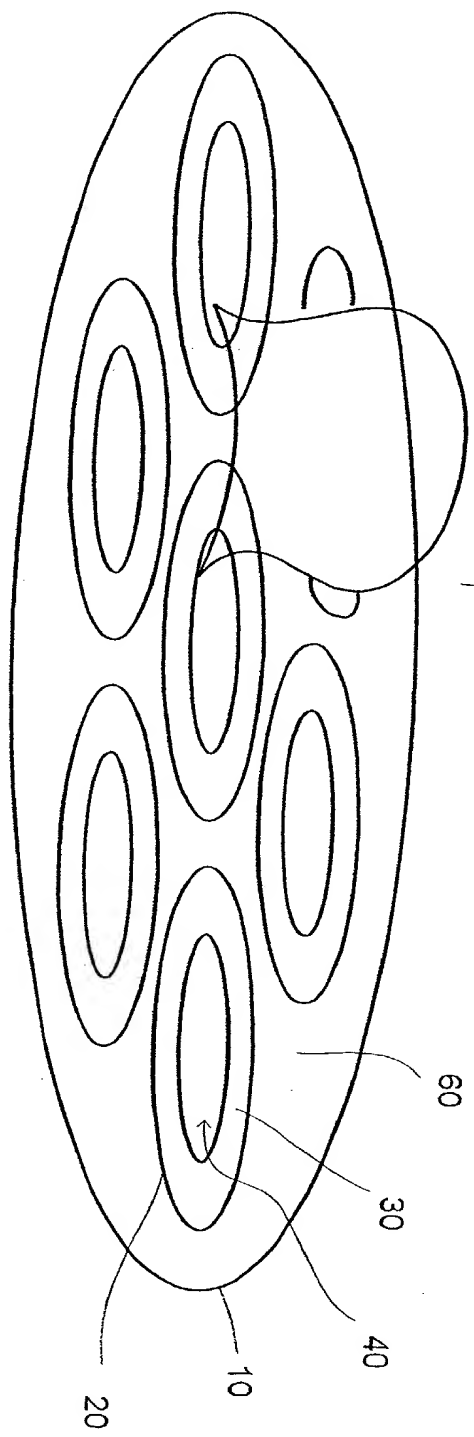


FIG. 7A



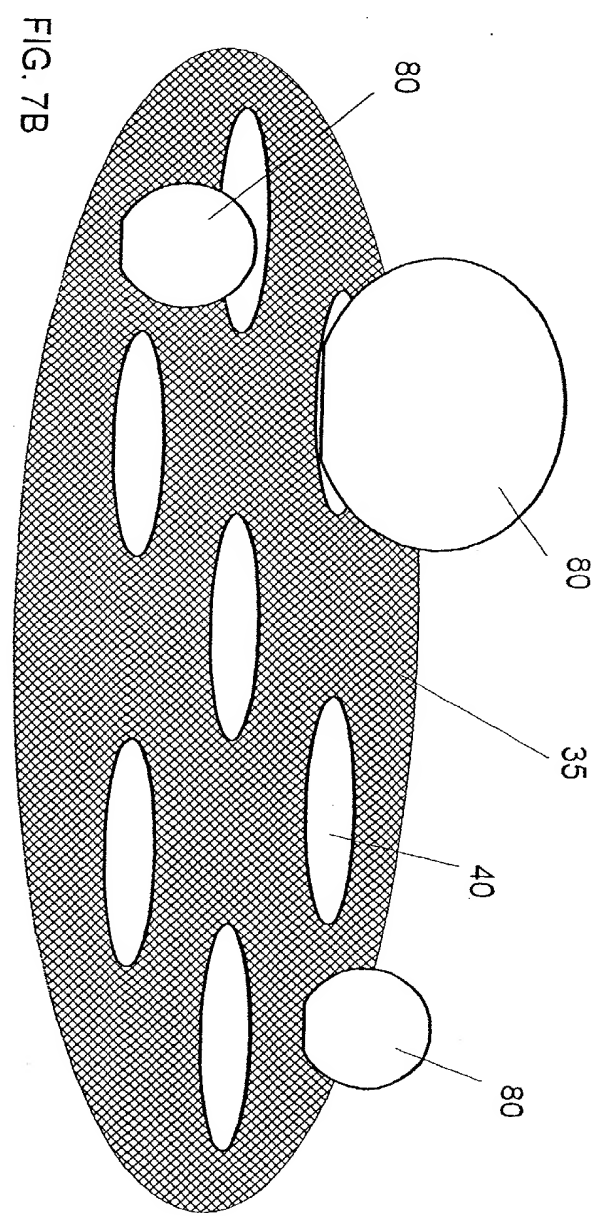



FIG. 7B

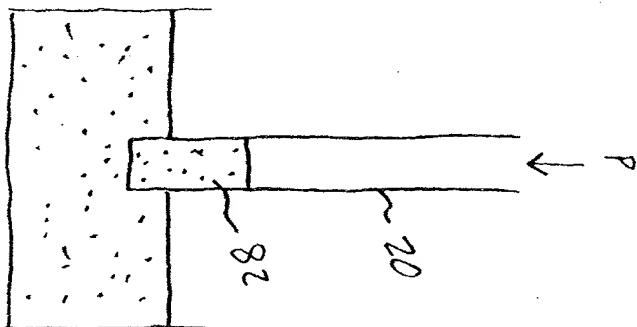

A.

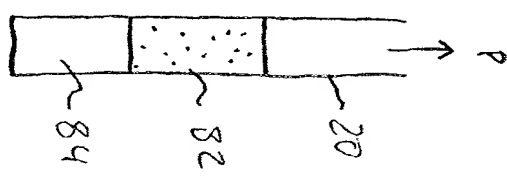

B.

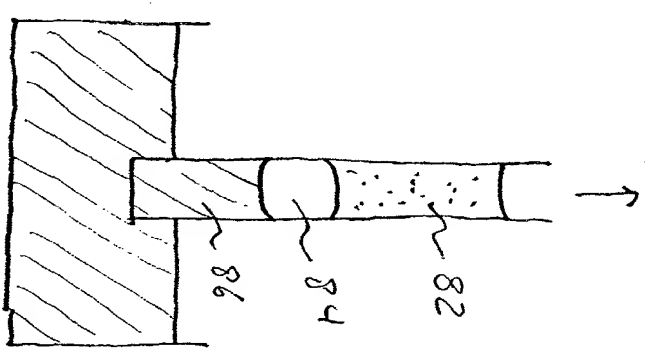

C.

FIG. 8

102290 95646860

Capillary array.

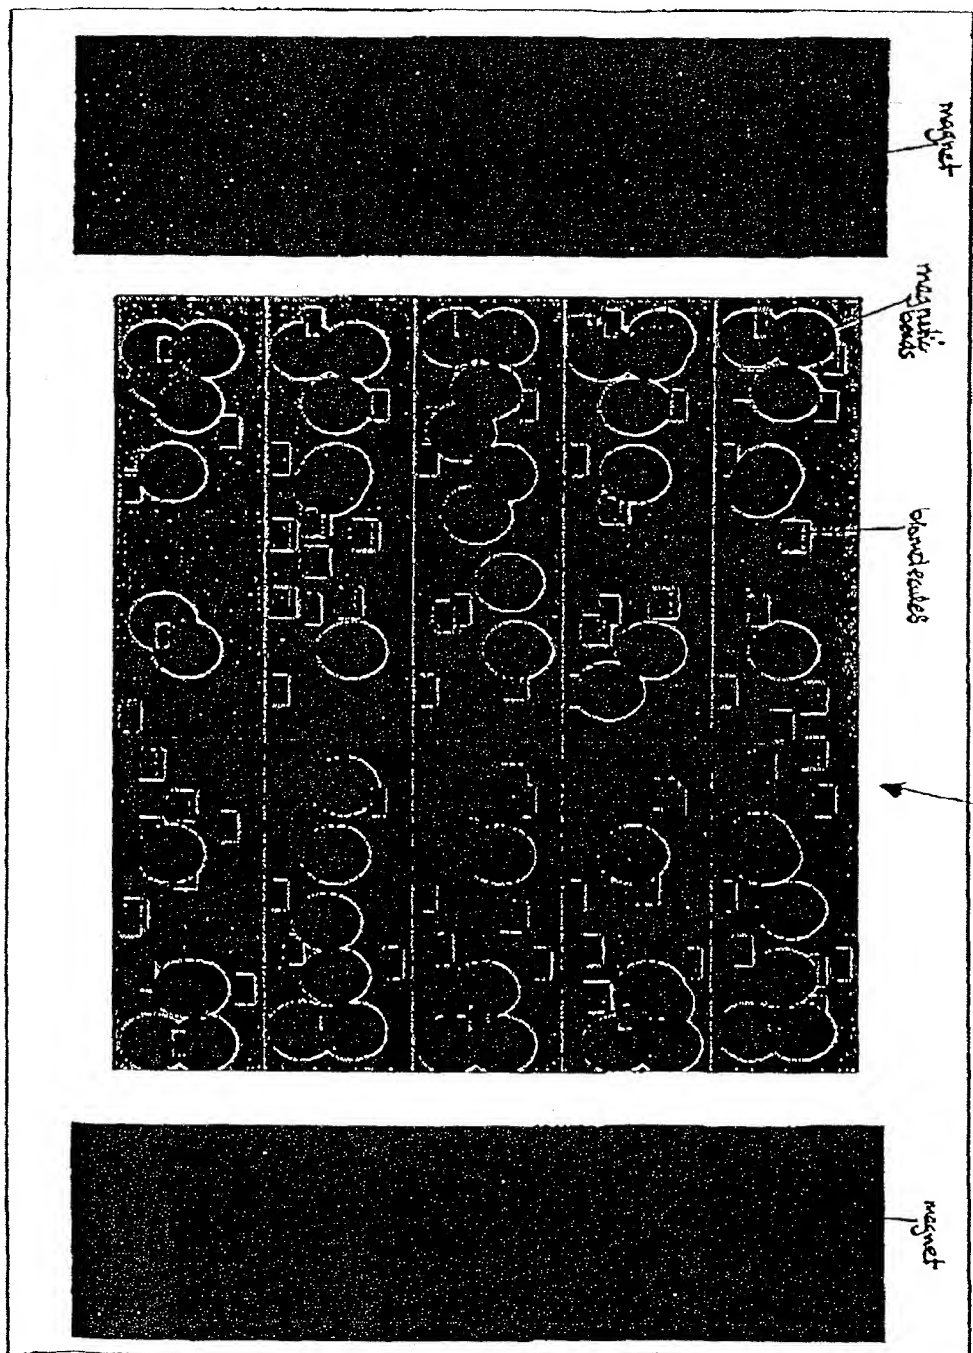


FIG. 9A

102290 95646860

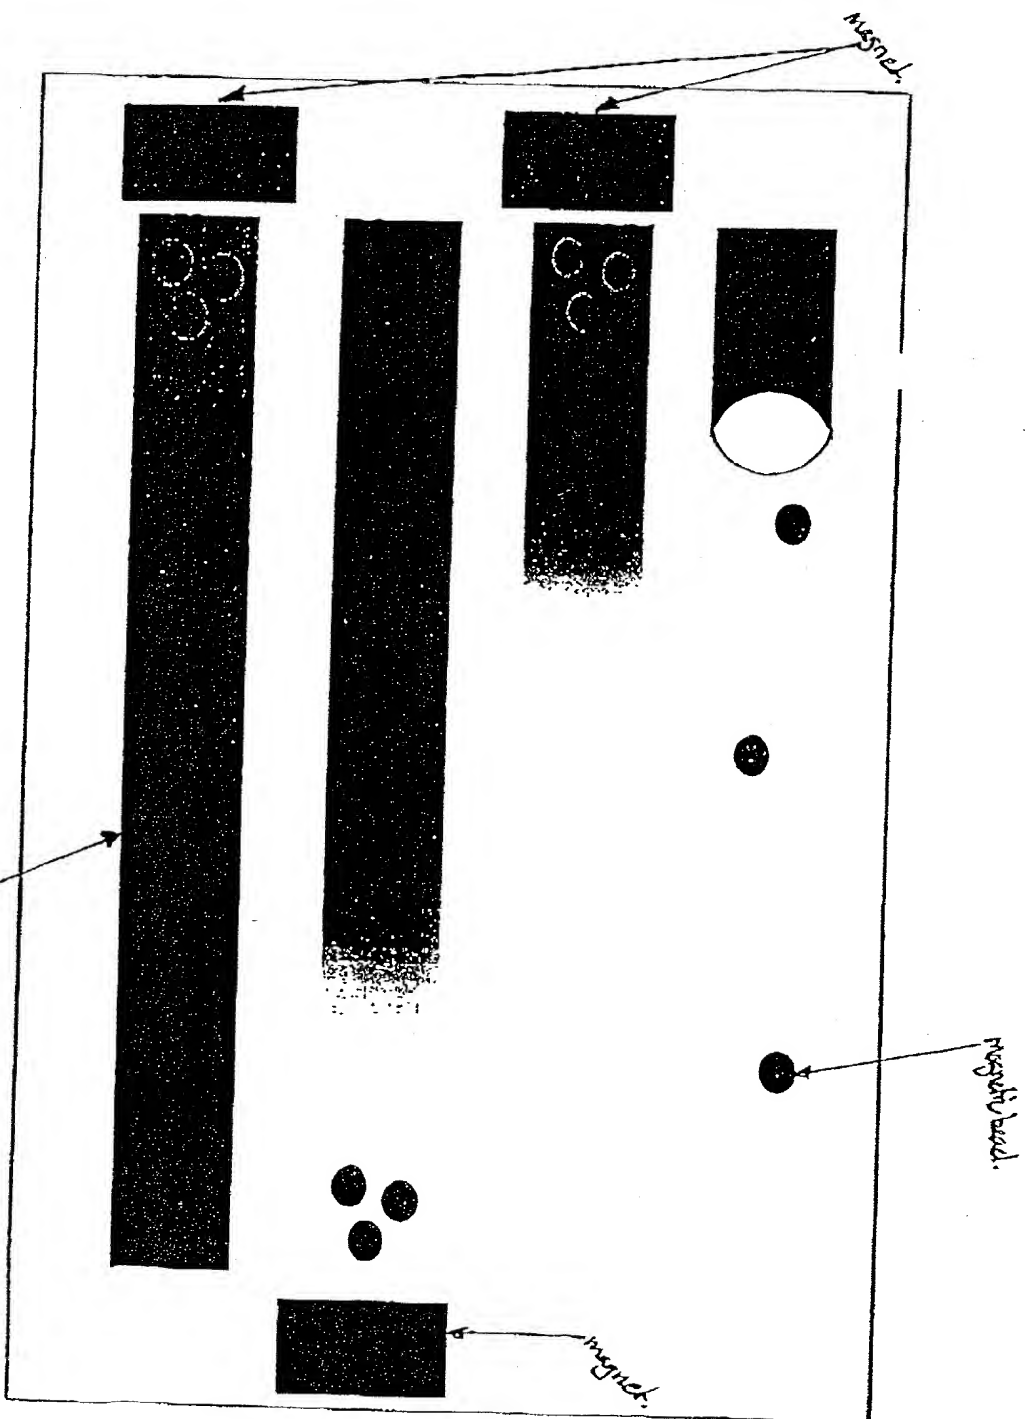


FIG. 9B

09894936 062701
T02290 95646860


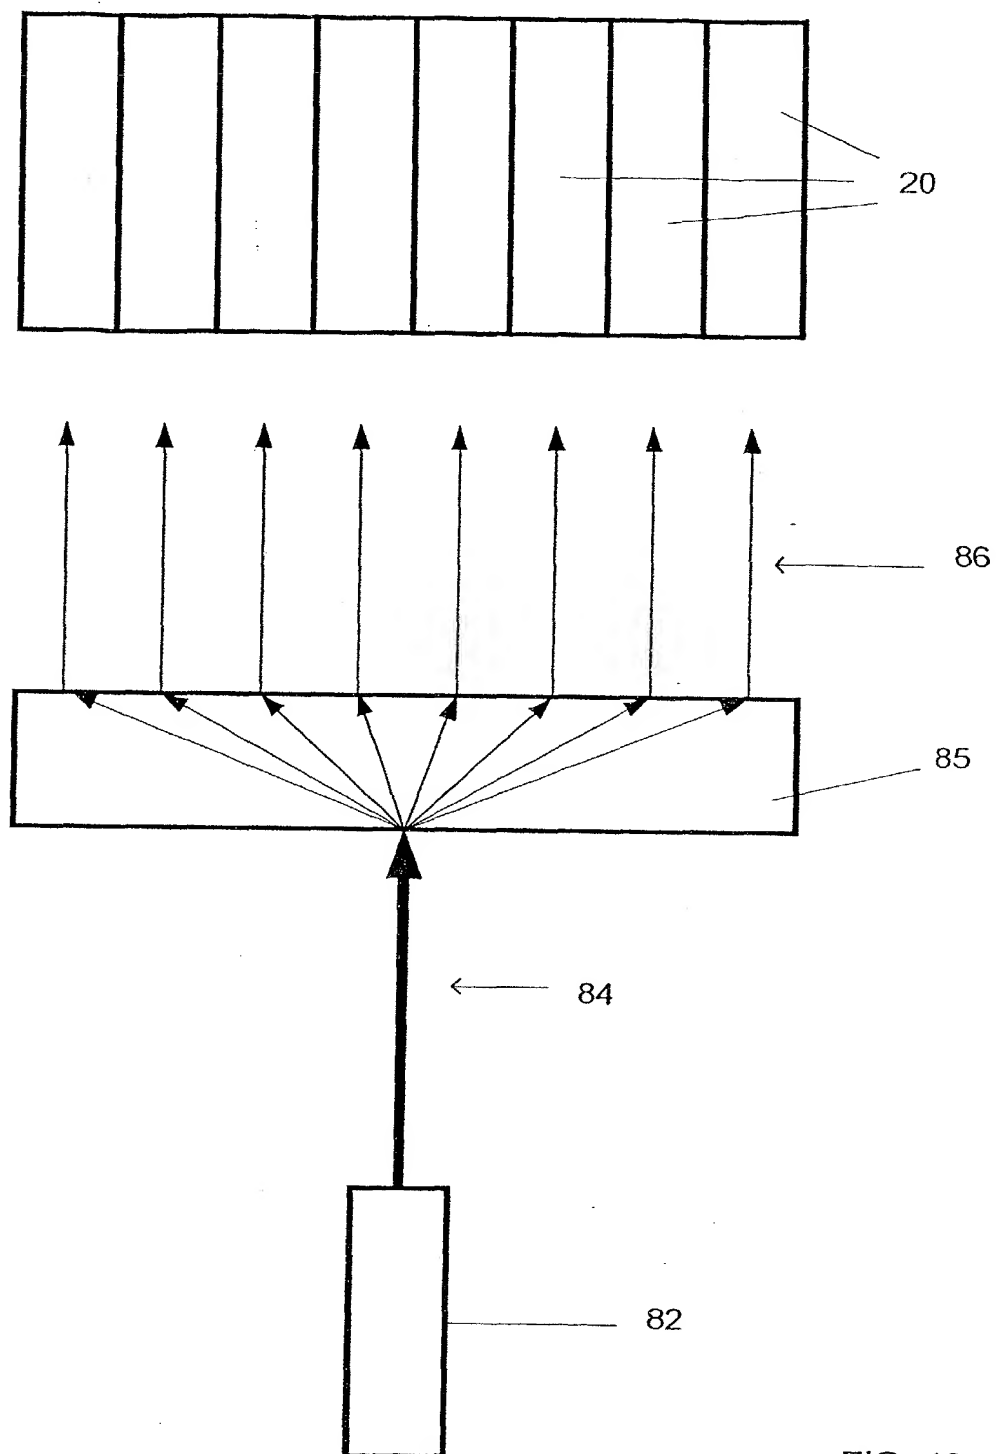


FIG. 10


Automated Hit Detection & Recovery System

FIG. 11


100

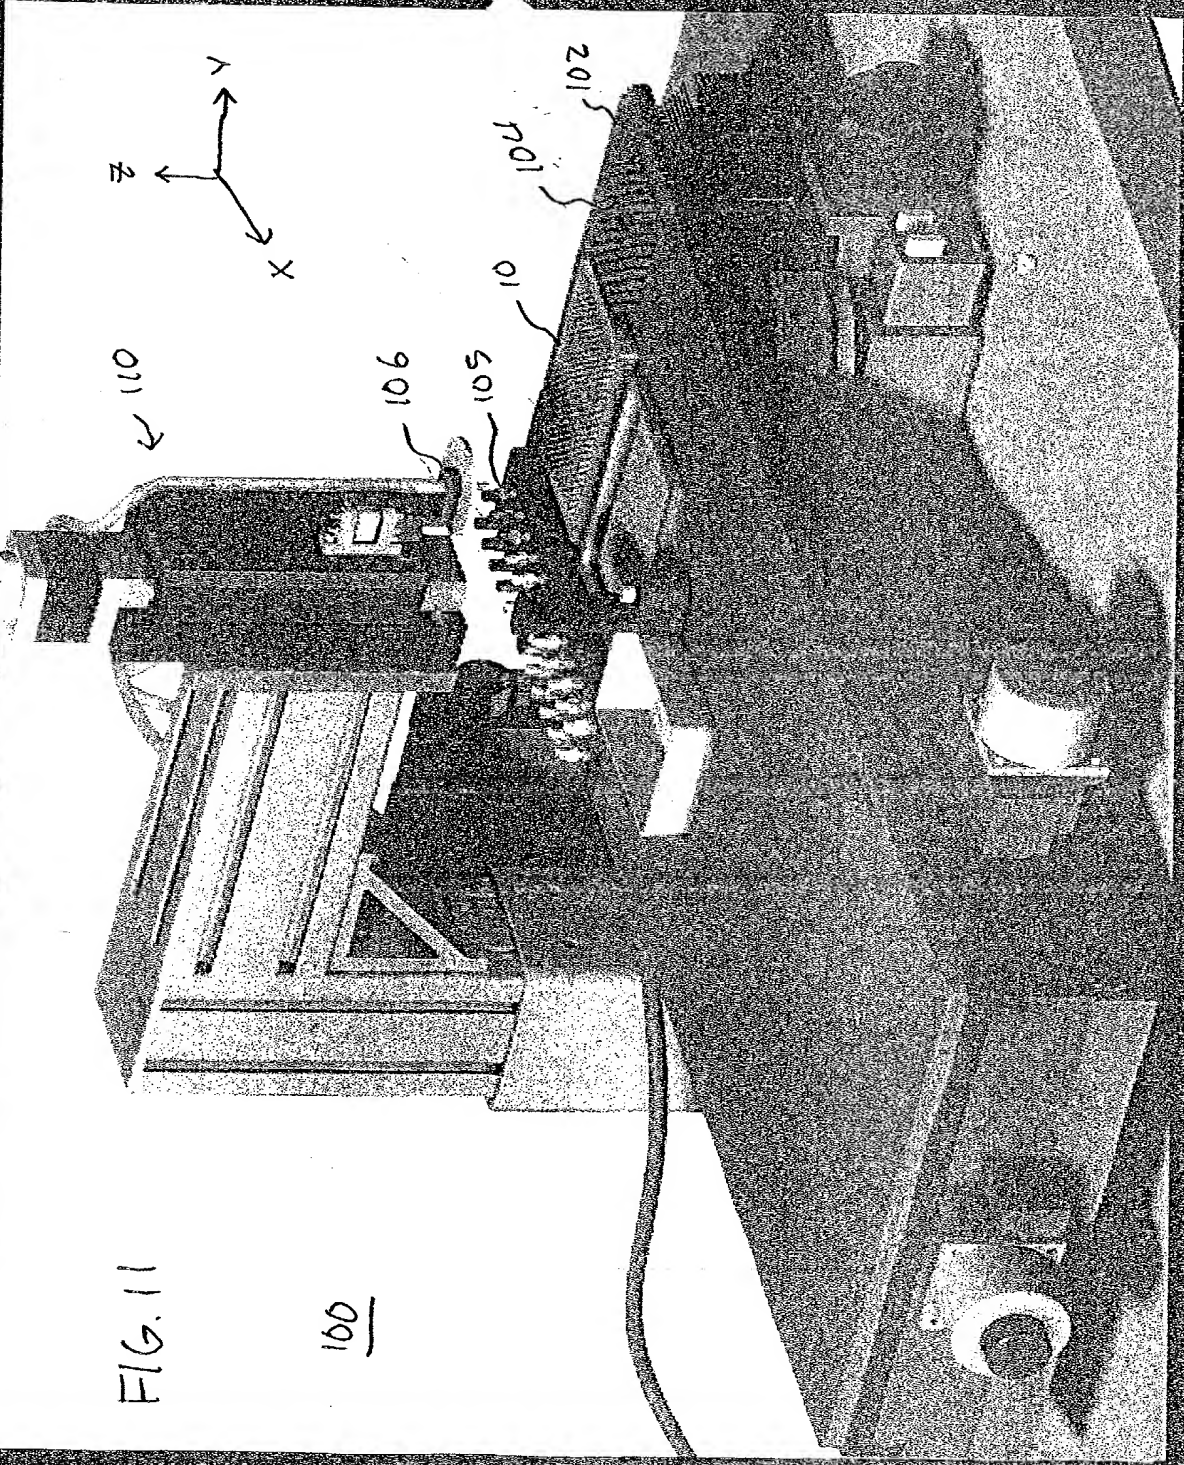

05894956 .062701

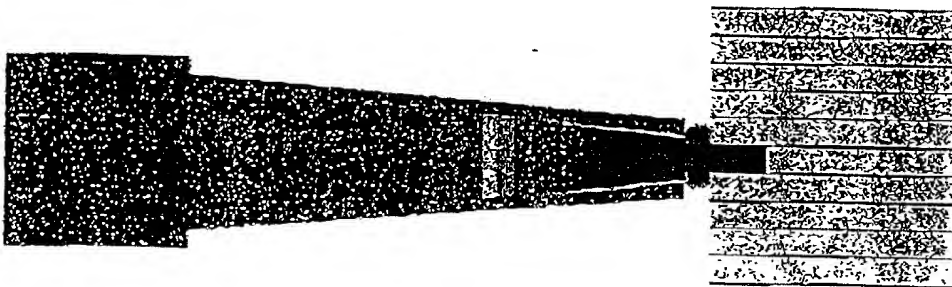

A

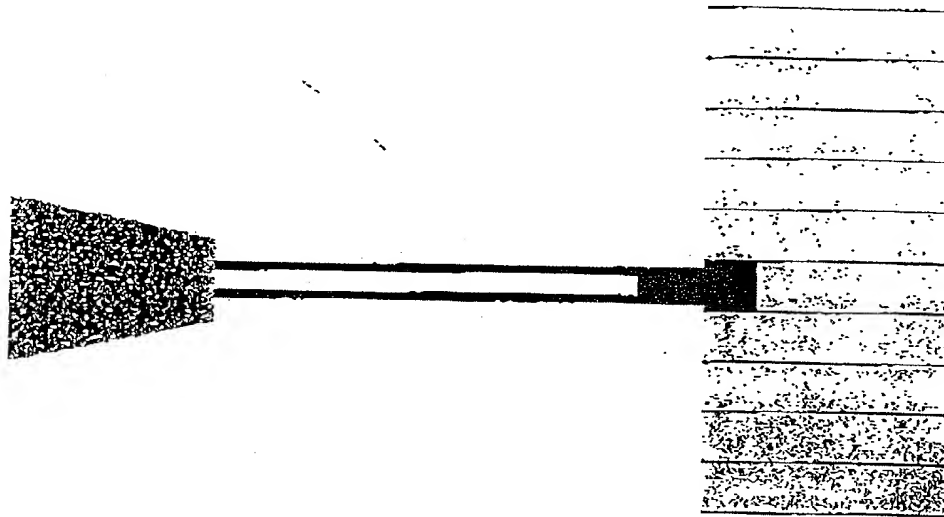

B

FIG. 12

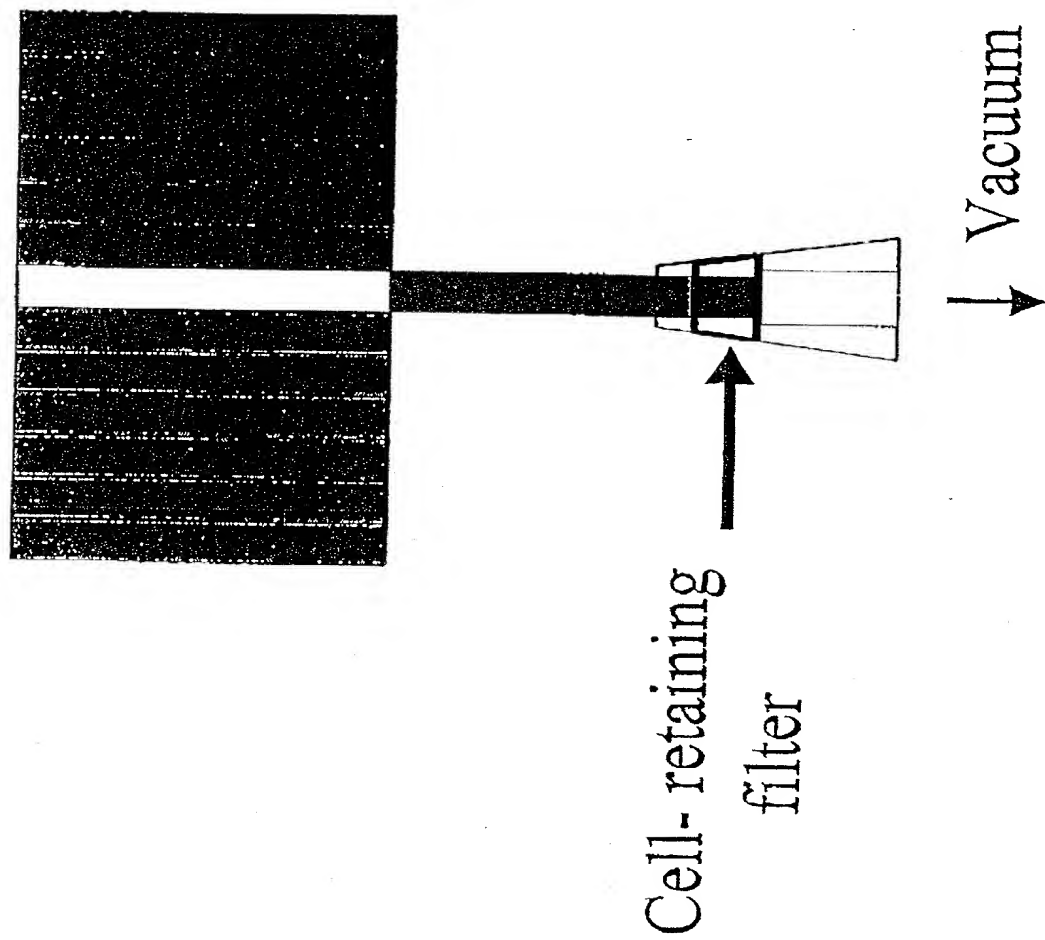


FIG. 12C

TO/290" 95646860

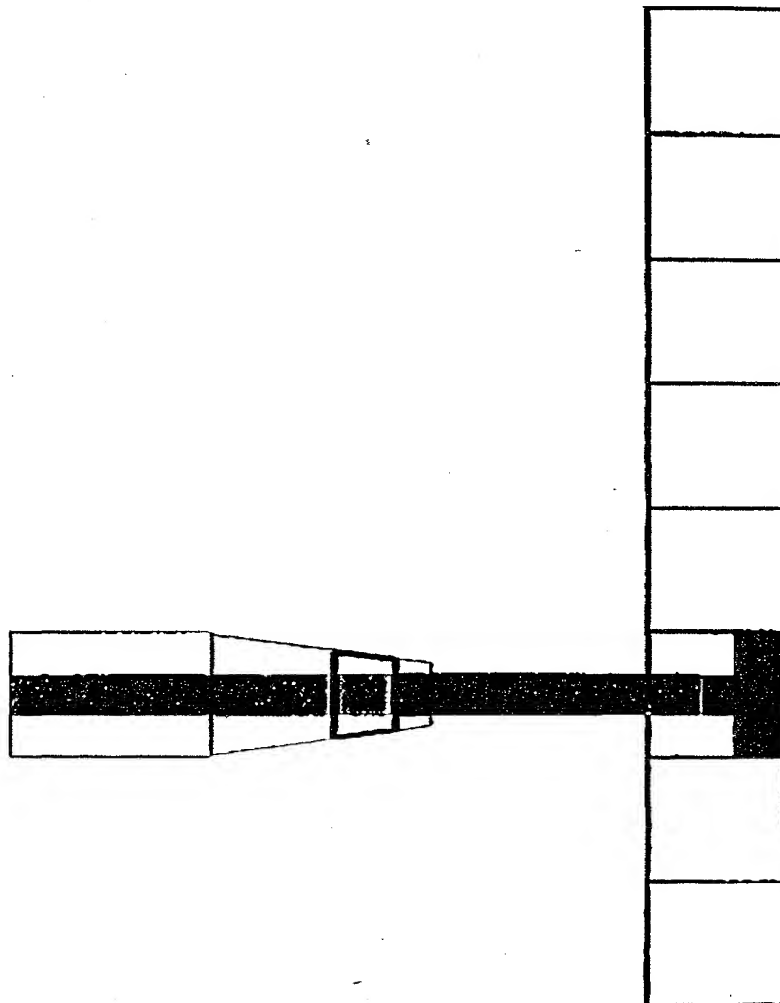


FIG. 12 D